



Solartron Metrology

SI3300

4-20mA/DC-Digital Display



The SI3300 is a member of the SI3000 Readout Family.
All members of the family are marked SI3000 on the front panel.

This manual is specifically for the SI3300 Model with 4-20mA/DC Voltage Inputs

user and installation manual

Index

Section	Title	Page
1.0	Index	1
2.0	Safety Summary	2
	Warnings and Cautions	2
3.0	Service and Repair	4
4.0	Bench Mounted or Installed into a Panel	5
4.1	Bench Mounted with associated Solartron Probes and power supply	5
4.2	Panel Mounting	6
4.3	Panel Dimensions	7
4.4	Assembly Dimensions	8
5.0	Display Panel	9
5.1	Layout of Front Panel	9
5.2	Layout of Rear Panel	10
5.3	Overview of Features	11
6.0	Operating Screen	13
6.1	MENUS and SETUPS	14
6.2	Probe Menu Channel A	15
6.3	Probe Menu Channel B	16
6.4	Measurement Menu Page 1	17
6.5	Measurement Menu Page 1 (cont.)	18
6.5.1	Measurement Menu Page 1 (cont.)	19
6.6	Measurement (Distance) Menu Page 2	20
6.7	Measurement (Angle) Menu Page 2	21
6.8	Limit Menu	22
6.9	Input/Output Menu	23
6.10	Serial Port Menu	24

Index

Section	Title	Page
6.11	Display Menu Screen 1	25
6.12	Display Menu Screen 2	26
6.13	Utilities Menu	27
6.14	Password Menu	28
6.15	Password Entry	29
6.16	Utilities Menu (Factory Default Restore)	30
6.17	Operator Screen	31
6.18	X Y Mode	32
6.19	Logging Menu Page 1	33
6.20	Logging Menu Page 2	34
7.0	RS232 User Input Commands	35
7.1	RS232 User Input Command Details	36
7.1	RS232 User Input Command Details (cont.)	37
7.1	RS232 User Input Command Details (cont.)	38
7.2	RS232 Output Formats	40
8.0	Interface Connections	41
8.1	I/O Connector	41
8.2	Communications Connector RS232	42
8.3	Power Connector	42
8.4	Analogue Voltage and Current Inputs	43
9.0	Technical Specifications	44

Return Of Goods

Solartron Sales Offices

2.0 Safety Information

Terms in this Manual

WARNING statements identify conditions or practices that could result in personal injury or loss of life.

CAUTION statements identify conditions or practices that could result in damage to the equipment or other property.

Symbols in this Manual



This symbol indicates where applicable cautionary or other information is to be found.

Service Safety

This equipment has been designed and tested to meet the requirements of the Low Voltage Directive (1997) and has been supplied in a safe condition. This manual contains information and warnings that must be followed by the user to ensure safe operation and to retain the apparatus in a safe condition.

Power Source

24v +/-10% DC 0.625A

2.0 Safety Information (cont.)

WARNINGS:

Do not operate in an explosive atmosphere

Do not remove covers or panels

To avoid personal injury, do not remove covers and panels. Do not operate the equipment without the covers and panels fitted. There are no internal adjustments required during commissioning of the equipment.

Grounding the Equipment

The unit is supplied by 24V DC and therefore does not require an earth grounding cable to avoid electric shock. However it is recommended that the unit is properly grounded to a known good earth via the bolt at the rear of the SI3300 to meet the full specification and EMC requirements.

3.0 Service and Repair

This equipment contains no user serviceable parts.

This equipment must be returned to your Solartron dealer for any service and repair.

The SI3300 is designed to be maintenance free. Contact with solvents should be avoided. Any attempt to dismantle the SI3300 will invalidate the warranty.

The SI3300 is a precision instrument and should be handled with care.

4.0 Bench Mounted or Installed into a Panel

4.1 Bench Mounted with associated Solartron Probes and power supply



4.0 Bench Mounted or Installed into a Panel (cont.)

4.2 Panel Mounting

- Ensure that there is sufficient space behind the relevant instrument panel for the SI3300 and its cabling (refer to section 4.3 for dimensions).
- Cut out the panel aperture to the dimensions shown.
- Working from behind the panel, with the box fully located, fit the side brackets to the studs and slide them forward toward the panel until they lock into place.
- Screw the brackets to the panel.

CAUTION: Do not over tighten the screws as this may damage the case of the instrument.

WARNING: On installing or removing the SI3300, you must be aware of any hazardous equipment or materials in the vicinity. Make sure that any equipment into which the SI3300 system is to be installed is switched off and made safe.


CAUTION: Avoid installing the SI3300 close to switch gear, contactors or motor starters.

CAUTION: Do not place other signal and power supply wiring in the same loom as the SI3300 wiring.

CAUTION: Use screened cables for all leads, with the screen earthed at one end only.


4.0 Bench Mounted or Installed into a Panel (cont.)

4.3 Panel Dimensions

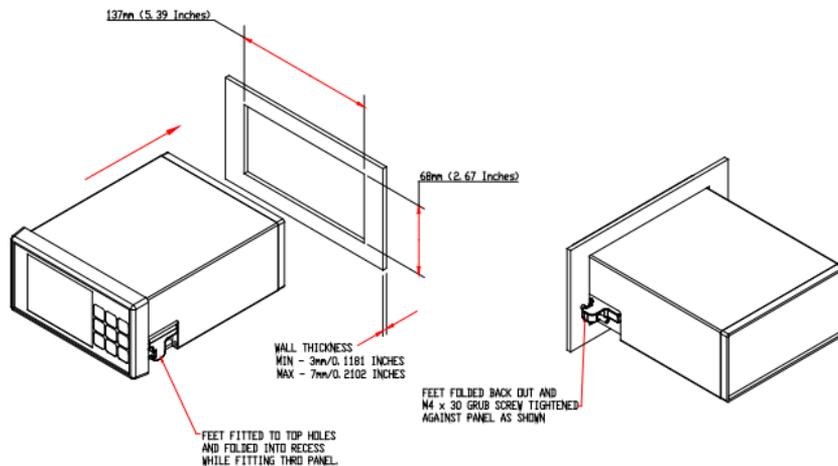

4.0 Bench Mounted or Installed into a Panel (cont.)

4.4 Assembly Dimensions

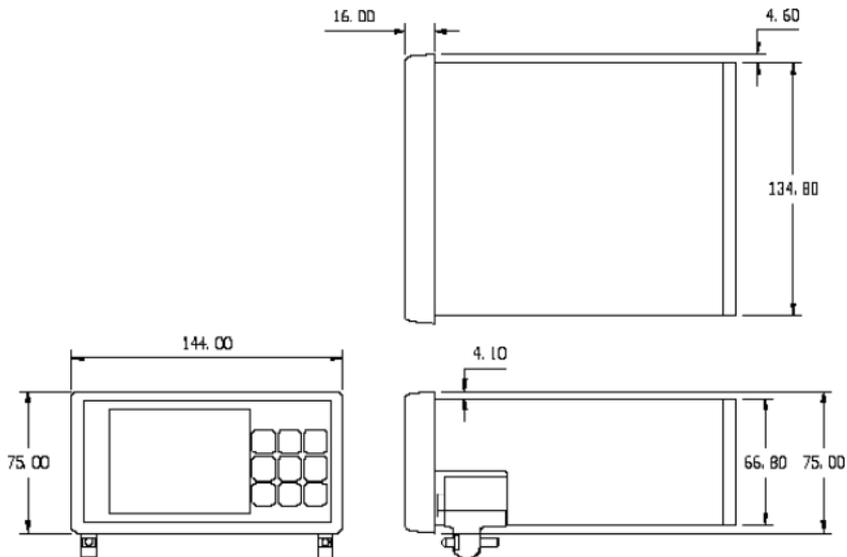

5.0 Display Panel


5.1 Layout of Front Panel



- 1 Liquid Crystal Operator Colour Display
- 2 Return to Setup Menu
- 3 Scroll Up (Moves cursor around screen), Apply Preset (ABS/PRE)
- 4 Print Option
- 5 Enter
- 6 Scroll Right (select option)
- 7 Track, Peak+, Peak-, Diff
- 8 Scroll Down (Moves cursor around screen)
- 9 Zero (ABS/TARE)
- 10 Scroll Left (select option)

5.0 Display Panel (cont.)

5.2 Layout of Rear Panel

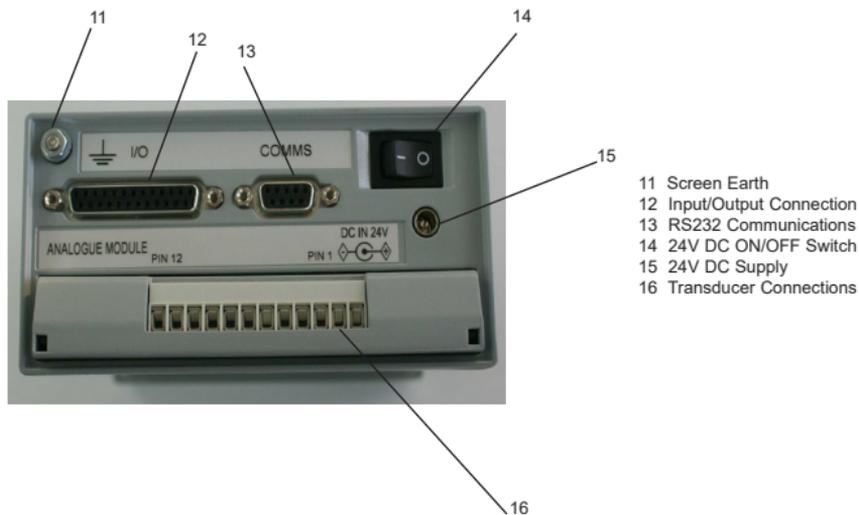

5.0 Display Panel (cont.)

5.3 Overview of Features

Transducers	<p>1 or 2 transducers may be connected SI3100 Series LVDT (Note: when setting up LVDT enter sensitivity in mV/V/mm regardless of final choice of measurement units) SI3300 Series 4-20 mA or DC inputs (0-5 V, 0-10 V, ± 5 V, ± 10 V)</p> <p>SI3500 Series – Orbit (Digital Probes and Linear Encoders)</p>																												
Measurements and Display	<p>The SI3000 series can display in single measurement mode A, B, A+B, A-B, (A+B)/2, (A-B)/2 and (B-A)/a</p> <p>The SI3300 and SI3500 series can display in dual measurement mode the sensor information A and B only; it is not possible to display any combinational information in dual display mode.</p> <p>(Note: (B-A)/a limited to ± 2.5 deg.)</p>																												
Limits	<p>Upper and lower limits are set for each individual measurement channel (A and B) and for a combinational measurement (e.g. A+B)</p> <p>The SI3000 series has 6 isolated open collector limit outputs which are allocated in accordance to the measurement mode.</p> <table border="1" data-bbox="295 632 1320 723"> <thead> <tr> <th></th> <th>Lower</th> <th>Good</th> <th>Upper</th> <th>Lower</th> <th>Good</th> <th>Upper</th> </tr> </thead> <tbody> <tr> <td>A</td> <td>Active</td> <td>Active</td> <td>Active</td> <td>Off</td> <td>Off</td> <td>Off</td> </tr> <tr> <td>B</td> <td>Off</td> <td>Off</td> <td>Off</td> <td>Active</td> <td>Active</td> <td>Active</td> </tr> <tr> <td>A+B etc</td> <td>Active</td> <td>Active</td> <td>Active</td> <td>Active</td> <td>Active</td> <td>Active</td> </tr> </tbody> </table> <p>If the measurement is within limit, then the good limit output is set, otherwise the upper or lower limit outputs are set to indicate a reading out of limit.</p>		Lower	Good	Upper	Lower	Good	Upper	A	Active	Active	Active	Off	Off	Off	B	Off	Off	Off	Active	Active	Active	A+B etc	Active	Active	Active	Active	Active	Active
	Lower	Good	Upper	Lower	Good	Upper																							
A	Active	Active	Active	Off	Off	Off																							
B	Off	Off	Off	Active	Active	Active																							
A+B etc	Active	Active	Active	Active	Active	Active																							

5.0 Display Panel (cont.)

5.3 Overview of Features (cont.)


Functions	<p>The SI3000 series has the following functions available from the front panel keypad or controllable from the RS232 and some discrete inputs.</p> <p>Zero: Allows a reading to be set to zero (display shows TARE) all measurements are then referenced to the zero position.</p> <p>Print: Allows measured data to be printed via the RS232 port.</p> <p>Peak/Track Allows the readout to be switched from track mode to peak+ or peak-. In peak mode the displayed value will only change if it is greater than (peak+) or less than (peak-) the current displayed value.</p> <p>Menu (keypad only) accesses menu screens for set up.</p> <p>The SI3300 and SI3500 series have the following additional functions:</p> <p>Preset: Allows a preset value to be added to the displayed reading only – does not change the analogue outputs. Enable preset from the preset menu and activate with the up arrow key.</p> <p>In dual display mode it is possible to set the preset and zero to activate on both channels.</p> <p>Log Mode: The readout can log and store data in three modes</p> <p>Normal logging which will store a number of readings at a predefined interval. Setup and start from logging menu screen</p> <p>Trigger start which will store a number of readings at a predefined interval, once the start logging input is triggered.</p> <p>Log on Trigger which will store a reading every time the logging input is triggered, this mode is started from the logging menu.</p>		
Inputs	6 discrete inputs, Zero, Change from track to peak+ to peak-, print, log, real reset, preset.		
Analogue Outputs	Analogue Output 1		Analogue Output 2
	A	A	Off (null)
	B	Off (null)	B
	A+B etc.	A+B etc.	A+B etc.
	Dual Display (SI3500 and SI3300 only)	A	B
Each analogue output can be independently set for 4-20 mA or a DC voltage (0-5 V, 0-10 V, ± 5 V and ± 10 V)			

6.0 Operating Screen

Display seen directly after powering up

Note: This screen will vary depending on the Operator Screen displayed prior to powering down

Press MENU go to 6.1

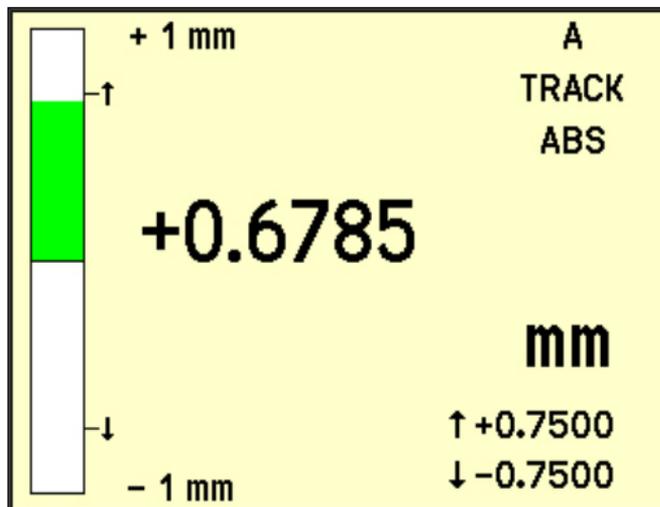

6.0 Operating Screen (cont.)

6.1 MENUS and SETUPS

Scroll up or down using the Δ ∇ keys to the required sub menu PRESS (ENTER)

Probes 6.2

Selects the type of probes to be used with this instrument, the parameters, channels and Identification associated with each probe.

Limits 6.8

Sets up the Upper and Lower measurement limits

Serial Port 6.10


Sets up the parameters for the Serial RS232 Port.

Utilities 6.13

Restore Factory Default Settings

Exit Menu 6.17

Shows Operator Screen

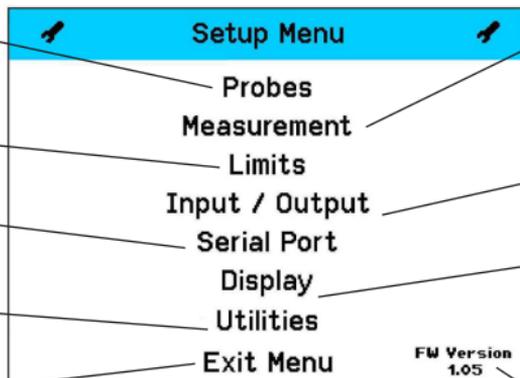

Measurement 6.4

Selects Measurement type. A,B,(A+B) etc.
Measurement Mode (Track, Peak+, Peak-, Diff)
Reset Mode (Manual/Auto)
Trigger Time (0000 ms)
Peak Trigger Level (+/-000.00000xx)
Units (mm,inch for distance)(rad,deg for angle)
Unipolar/Bipolar (Auto Mode, Unipolar, Bipolar)
Distance 'n' (0001.0000) for angle

Input/Output 6.9

Logic I/O + Analogue outputs
Print options

Display 6.12

Set Language, Contrast,
Bar Offset, Bar
(+/-000.00000)
AutoRange (on/off)
Places After Decimal
point (0 to 6)


Shows current
Firmware version

6.0 Operating Screen (cont.)

6.2 Probes Channel A

Use \triangle ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.
e.g. Extend + or Retract-

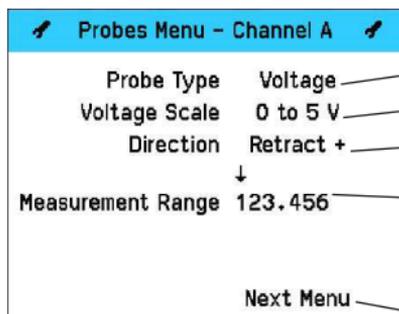

- \triangleleft \triangleright NONE, Voltage, Current
- \triangleleft \triangleright 4-20mA, 0-5V, 0-10V, +/-5V, +/-10V
- \triangleleft \triangleright EXTEND +
- \triangle ∇ Press ENTER to Edit parameter
- \triangleleft \triangleright To move cursor
- \triangle ∇ To increment/decrement numbers
- \triangle ∇ To change +/-
Press ENTER to Exit Mode

Press ENTER see 6.3
Channel B

Notes

Press MENU to return to the Operator Screen

With cursor over NEXT MENU Press ENTER for next sub Menu

With cursor over EXIT MENU Press ENTER to return to Setup Menu

6.0 Operating Screen (cont.)

6.3 Probes Channel B

Use Δ ∇ to move the cursor around the screen.

Use \leftarrow \rightarrow to select options.
e.g. Extend + or Retract+

The screenshot shows the 'Probes Menu - Channel B' screen with the following text and callouts:

- Probe Type** Voltage: \leftarrow \rightarrow NONE, Voltage, Current
- Voltage Scale** 0 to 5 V: \leftarrow \rightarrow 4-20mA, 0-5V, 0-10V, +/-5V, +/-10V
- Direction** Retract +: \leftarrow \rightarrow EXTEND +
- Measurement Range** 123.456: Δ ∇ Press ENTER to Edit parameter
- Back** Exit Menu: \leftarrow \rightarrow To move cursor
- Back** Exit Menu: Δ ∇ To increment/decrement numbers
- Back** Exit Menu: Δ ∇ To change +/-
Press ENTER to Exit Mode
- Back** Exit Menu: Press ENTER see 6.1 Channel B

Notes

Press MENU to return to the Operator Screen

With cursor over BACK Press ENTER for previous sub Menu


With cursor over EXIT MENU Press ENTER to return to Setup Menu

6.0 Operating Screen (cont.)

6.4 Measurement Menu Page 1

Use \triangle ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.

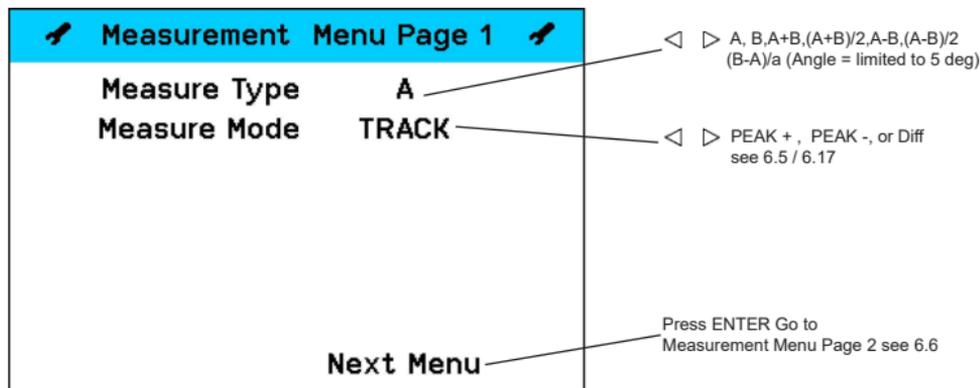

6.0 Operating Screen (cont.)

6.5 Measurement Menu Page 1

Use Δ ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.

Measurement Menu Page 1


Measure Type	A	\triangleleft \triangleright Measure Type B,A+B,(A+B)/2,A-B,(A-B)/2,(B-A)/a (Shows on Operator Screen in mm, inch for distance)
Measure Mode	PEAK+	\triangleleft \triangleright Measure Mode Track, Peak+, Peak-, Diff
Peak Reset Mode	Manual	\triangleleft \triangleright Auto, Manual Auto Mode only
Peak Trigger Time	12345	Δ ∇ Press ENTER to Edit parameter \triangleleft \triangleright To move cursor
Peak Trigger Level	+123.456789	Δ ∇ To increment/decrement numbers Δ ∇ To change +/- Press ENTER to Exit Mode
Next Menu		Press ENTER see 6.6

6.0 Operating Screen (cont.)

6.5.1 Measurement Menu Page 1

Use Δ ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.

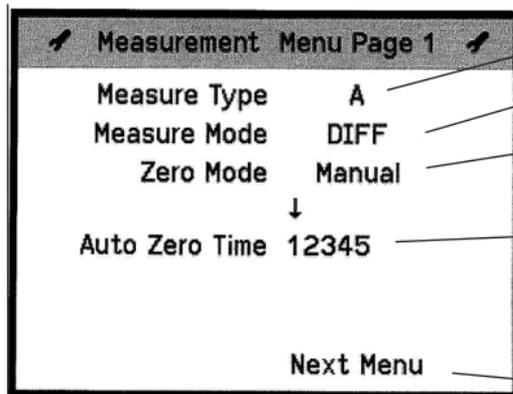

\triangleleft \triangleright Measure Type B,A+B,(A+B)/2,A-B,(A-B)/2, (B-A)/a
(Shows on Operator Screen in mm, inch for distance)
(Shows on Operator Screen in rad, deg for angle)

\triangleleft \triangleright Measure Mode Track, Peak+, Peak-, Diff

\triangleleft \triangleright Auto, Manual

Diff Mode only

Δ ∇ Press ENTER to Edit parameter

\triangleleft \triangleright To move cursor

Δ ∇ To increment/decrement numbers

Δ ∇ To change +/-
Press ENTER to Exit Mode


Press ENTER

6.0 Operating Screen (cont.)

6.6 Measurement Menu Page 2

Use \triangle ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.

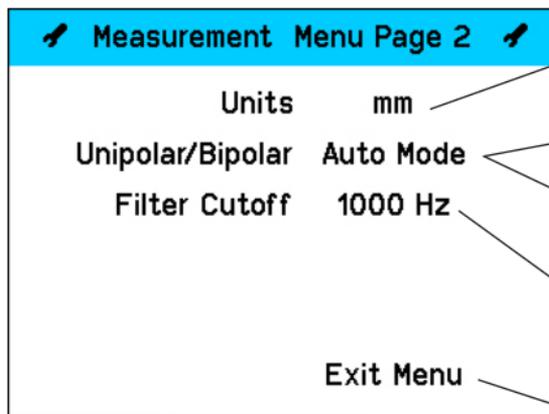

\triangleleft \triangleright mm, inches, none

\triangleleft \triangleright Bipolar, Unipolar or Auto Mode

Bipolar selected

Measurement range displayed Top + xx mm/inch

Bottom - xx mm/inch

Centrally Tracks the +/- measurements within limits in green turning to red when outside the limits.

Unipolar selected

Measurement range displayed Top + xx mm/inch

Bottom 0 xx mm/inch

Tracks the + measurement within limit turning to red when outside the limit.

Display filter 4 Hz, 8 Hz, 250 Hz, 1000 Hz

Press ENTER


Back to Setup Menu

6.0 Operating Screen (cont.)

6.7 Measurement (Angle) Menu Page 2

Use Δ ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.

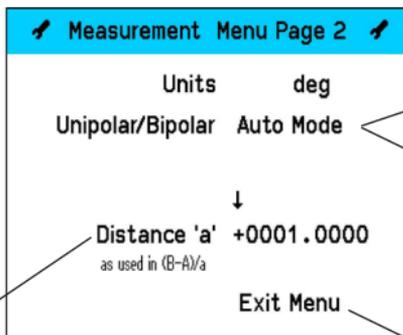

\triangleleft \triangleright Bipolar, Unipolar or Auto Mode

Bipolar selected

Measurement range displayed Top + xx rad/deg
Bottom - xx rad/deg

Centrally Tracks the +/- measurements within limits in green turning to red when outside the limits.

Unipolar selected

Measurement range displayed Top + xx rad/deg
Bottom 0 xx rad/deg

Tracks the + measurement within limit turning to red when outside the limit.

Press ENTER see 6.1
Back to Setup Menu

Auto Mode only

Δ ∇ Press ENTER to Edit parameter

\triangleleft \triangleright To move cursor

Δ ∇ To increment/decrement numbers


Δ ∇ To change +/-
Press ENTER to Exit Mode

6.0 Operating Screen (cont.)

6.8 Limit Menu

Use Δ ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.

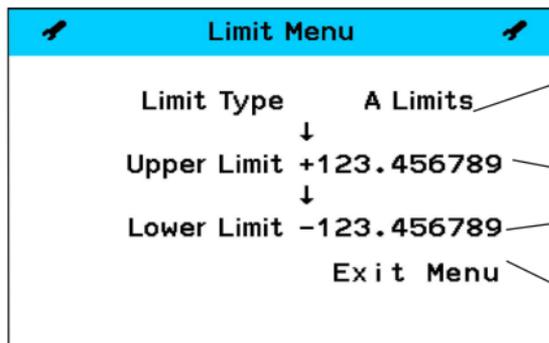

3 types of limits can be displayed A,B and "Computed Limits" when more than one measurement type selected see 6.4

- Δ ∇ Press ENTER to Edit parameter
- \triangleleft \triangleright To move cursor
- Δ ∇ To increment/decrement numbers
- Δ ∇ To change +/-
Press ENTER to Exit Mode

Press ENTER see 6.1
Back to Setup Menu

6.0 Operating Screen (cont.)

6.9 Input/Output Menu

Use \triangle ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.

The screenshot shows the 'Input/Output Menu' with the following items and their corresponding options:


Item	Option	Callout
Logic Inputs	Active Low	\triangleleft \triangleright Active High
Logic Outputs	Active Low	\triangleleft \triangleright Active High
Analogue O/P Ch A	0 to 5 V	\triangleleft \triangleright 0 to 10V, -5 to +5V -10 to +10V 4-20mA
Analogue O/P Ch B	0 to 5 V	\triangleleft \triangleright 0 to 10V, -5 to +5V -10 to +10V 4-20mA
Print Button Options	Single	\triangleleft \triangleright Continuous
Print Discrete Options	Single	
Exit Menu		Press ENTER see 6.1 Back to Setup Menu

6.0 Operating Screen (cont.)

6.10 Serial Port Menu

Use \triangle ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.

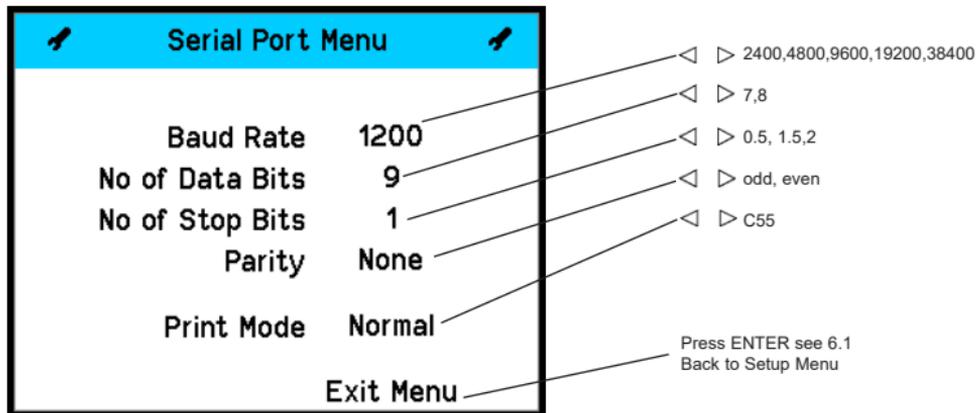

6.0 Operating Screen (cont.)

6.11 Display Menu - Screen 1

Use \triangle ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.

Varies the screen contrast for optimum operator viewing screen

Offsets bar + or -

Switches Bar Auto Range On/Off

Sets places after Decimal Point
This needs to be set separately for CHA, CHB + Computed Measurement (A+B, A-B etc.)

Press ENTER see 6.1 for next menu

Display Menu Page 1	
Language	English
Contrast	50
↓	
Bar Offset	+0000.0000
Bar AutoRange	Off
Places After DP	0
Next Menu	Exit Menu

\triangleleft \triangleright 0,5,10,15,20,25,30,35,40,45,50,55,60,65,70,75,80,85,90,95,100

\triangle ∇ Press ENTER to Edit parameter

\triangleleft \triangleright To move cursor

\triangle ∇ To increment/decrement numbers

\triangle ∇ To change +/-
Press ENTER to Exit Mode

\triangleleft \triangleright On

\triangleleft \triangleright 1,2,3,4,5,6


Press ENTER see 6.1
Back to Setup Menu

6.0 Operating Screen (cont.)

6.12 Display Menu - Screen 2

Use Δ ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.

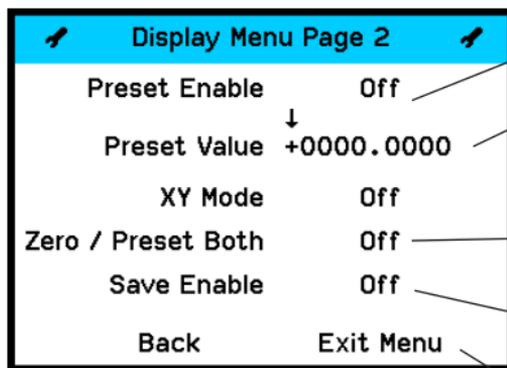

Use \triangleleft \triangleright On, Off

Δ ∇ Press ENTER to Edit number

Δ ∇ To move cursor

Δ ∇ To increment/decrement number

Δ ∇ To change +/-
Press ENTER to Exit Mode

Use \triangleleft \triangleright On, Off (see section 6.18)

\triangleleft \triangleright Off/Zero/Preset/Both
Option to save Zero, Preset or Both


Δ Select Back/Exit Menu
Enter to Action
 ∇

6.0 Operating Screen (cont.)

6.13 Utilities Menu

Use Δ ∇ to move the cursor around the screen.

Use \triangleleft \triangleright to select options.

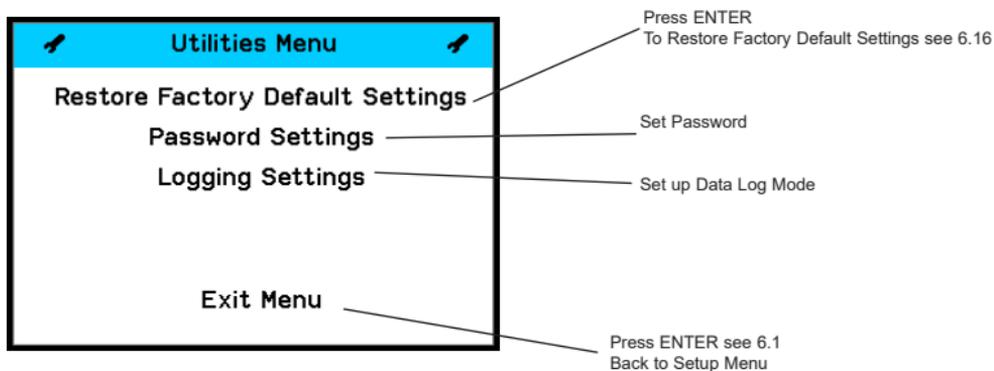


6.0 Operating Screen (cont.)

6.14 Password Menu

Use Δ ∇ to move the cursor around the screen.

Use \leftarrow \rightarrow to select options.

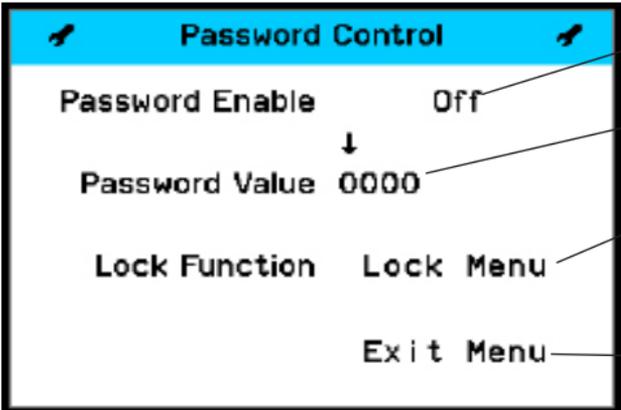

The screenshot shows a terminal-style interface for the Password Control menu. The title bar is blue with the text "Password Control" and two key icons. The menu items are:

- Password Enable Off
- ↓
- Password Value 0000
- Lock Function Lock Menu
- Exit Menu

Callouts provide the following information:

- Keys to turn On/Off (pointing to the "Off" status)
- Default set to 1234. Use ENTER and \leftarrow \rightarrow keys to change, Press ENTER to confirm (pointing to the "Password Value 0000")
- \leftarrow \rightarrow Lock Menu, Lock ALL. Note: If Lock ALL is applied all keypad functions are disabled except menu screen. (pointing to the "Lock Menu" option)
- Press ENTER see 6.1 Back to Setup Menu (pointing to the "Exit Menu" option)


6.0 Operating Screen (cont.)

6.15 Password Entry

Note: Only seen if password enabled

Use \triangle ∇ to move the cursor around the screen.


Use \triangleleft \triangleright to select options.

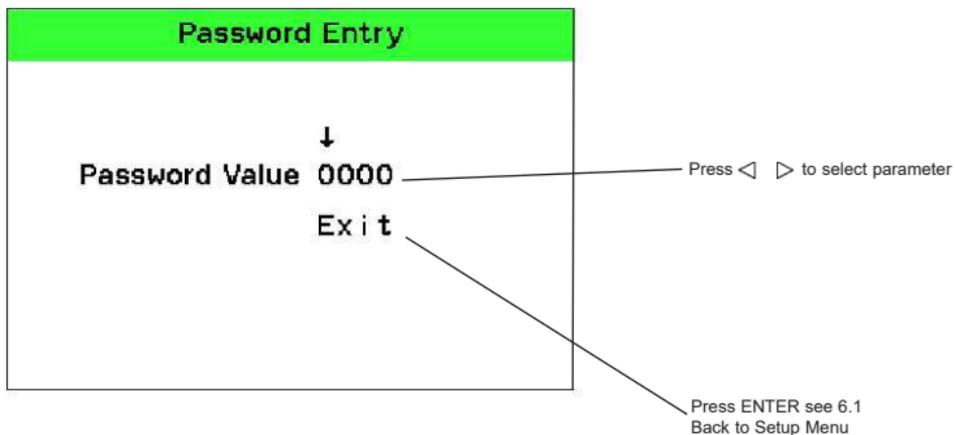

6.0 Operating Screen (cont.)

6.16 Utilities Menu (Factory Default Restore)

The following is displayed for 3 seconds, the unit automatically defaults to factory setting and returns to the Operator Screen.

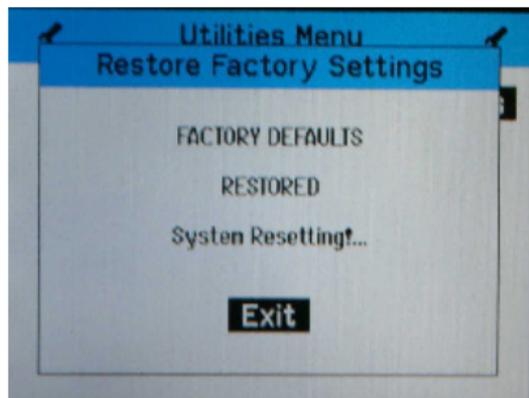

6.0 Operating Screen (cont.)

6.17 Operator Screen

The diagram shows a rectangular operator screen with a yellow background. On the left side, there is a vertical scale with a green bar indicating a measurement level. The scale has markings for +1 mm at the top and -1 mm at the bottom. The green bar is positioned between the 0 and +1 mm marks, with a small upward arrow above it and a downward arrow below it. The main display area shows the number **+0.6785** in large black font. To the right of this number, the word **TRACK** is displayed above **ABS**. Below these, the unit **mm** is shown. At the bottom right, there are two lines of text: **↑ +0.7500** and **↓ -0.7500**. A small letter **A** is located in the top right corner of the screen area. Several callout lines point to different parts of the screen with descriptive text.

Auto Range ON/OFF see 6.7 Display Menu

Selected Measurement Menu see 6.3

TRACK PEAK+,PEAK-,DIFF Selected at Measurement menu see 6.3 or PEAK/TRACK membrane on keypad
TRACK Measures actual distance/angle within the set limits displaying green. Turning red when outside the set limits. Returning to green when back inside the limits.

PEAK+ Measures within the set limits displaying green turning red when outside the set limits.
Pressing ENTER resets

PEAK- Measures within the set limits displaying green turning red when outside the set limits.
Pressing ENTER resets


DIFF measures Peak+, Peak-, measures within the set limits displaying green turning red when outside of limits out
If manual set, Peak +/- Press enter to reset.
If Auto set, Peak + reset to probe actual position
Below Peak Trigger Time/Peak Trigger Level
If Auto set, Peak - reset to probe actual position
Above Peak Trigger Time/Peak Trigger Level
If Auto set, Diff - Diff zeroed every time period

Press Zero to select ABS (Absolute) or TARE (Offset)

Selected by Limit Menu
Press MENU see 6.1 Set Up Menu

6.0 Operating Screen (cont.)

6.18 X Y Mode

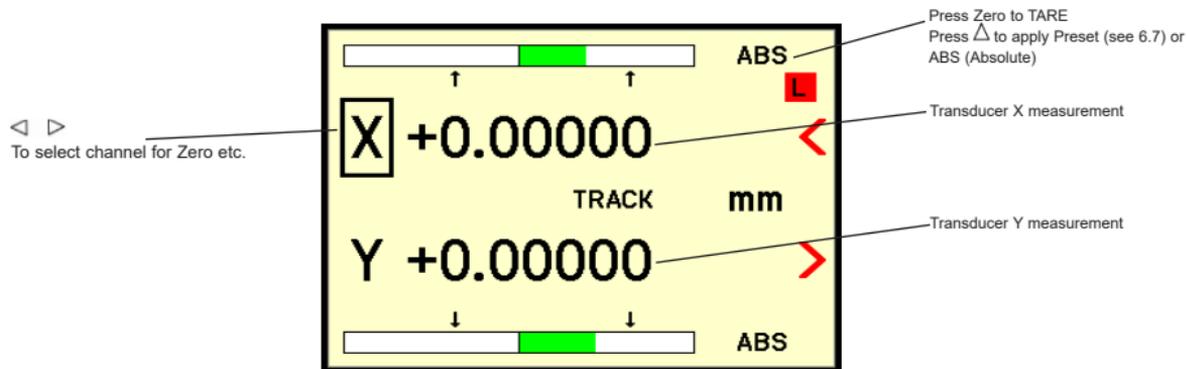

6.0 Operating Screen (cont.)

6.19 Logging Menu Page 1

The screenshot shows a menu titled "Logging Menu Page 1" with a blue header. The menu items are arranged in two columns:


Mode	Standard
Auto Summary	Off
Interval (ms)	000001000
Duration (ms)	000060000
Itemise	Off
Next Menu	Exit Menu

Navigation instructions:

- Use ◀ ▶ to select Standard, Start on Discrete Input or Trigger on Discreet Input
- Use ◀ ▶ to select On, Off
- Press ENTER to edit number
- ◀ ▶ To Move Count
- △ ▽ To Increment Number
- Press ENTER to Exit mode

6.0 Operating Screen (cont.)

6.20 Logging Menu Page 2

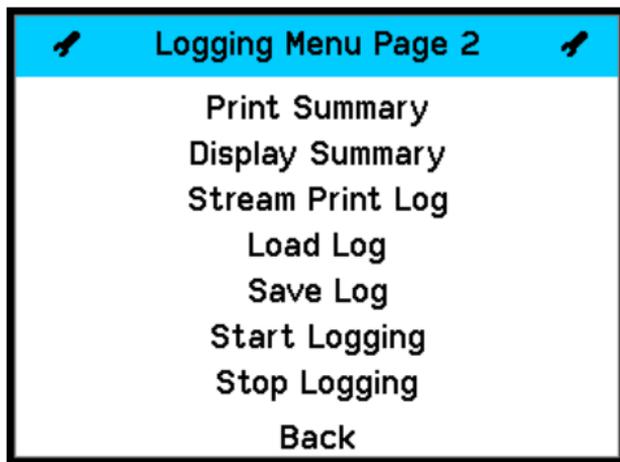

Use  to move to option


Press ENTER to Select option

7.0 RS232 User Input Commands

The unit shall respond to the following RS232 User Input Commands

Command	Command Sequence	Number of Parameter Bytes	Description
Print	""O'	0	Print Mode = Normal : Standard print Print Mode = C55 : C55 compatible print (Print Mode option is located in the 'serial port' menu)
Extended Print	""P'	1	Print in SI3300 Format
Get Detail	""E'	2	Return Details about the SI3300 <i>ABS or TARE, Measurement Type, Unit of Measure, Limit Values</i>
Set Unit	""S'	11	Set Various SI3300 Settings <i>Limits, Stroke, Measurement Type, Measurement Mode, Zero, Start/Stop Continuous Print, Set Print Button Mode, Notify, Stop Notify, Peak Reset, Discrete Inputs Active Hi/L0, Discrete Outputs Active Hi/L0</i>

Detailed Command specification with full parameter details follows on the next pages.

7.0 RS232 User Input Commands (cont.)

7.1 RS232 User Command Details

In the following table sp is used to mean an Ascii space (Dec 32 Hex 20)
Shaded cells mean they are not used for the command shown

Command	Total No of Chars	Character Number																	
		1	2	3	4	5	6	7	8	9	10	11	12	13					
Print	2	^	O																
Extended Print																			
<i>Current Measurement</i>	3	^	P	0															
<i>Channel A</i>	3	^	P	1															
<i>Channel B</i>	3	^	P	2															
GetDetail																			
<i>Get Abs or Tare</i>	4	^	E	A	0														
<i>Get Measurement Mode</i>	4	^	E	M	0														
<i>Get Unit of Measure</i>	4	^	E	U	0														
<i>Get Current Mode LL</i>	4	^	E	L	0														
<i>Get Current Mode UL</i>	4	^	E	L	1														
<i>Get Computed LL</i>	4	^	E	L	2														
<i>Get Computed UL</i>	4	^	E	L	3														
<i>Get Channel A LL</i>	4	^	E	L	4														
<i>Get Channel A UL</i>	4	^	E	L	5														
<i>Get Channel B LL</i>	4	^	E	L	6														
<i>Get Channel B UL</i>	4	^	E	L	7														
<i>Get Computed Stroke</i>	4	^	E	S	0														
<i>Get Channel A Stroke</i>	4	^	E	S	1														
<i>Get Channel B Stroke</i>	4	^	E	S	2														

7.0 RS232 User Input Commands (cont.)

7.1 RS232 User Command Details (cont.)

In the following table sp is used to mean an Ascii space (Dec 32 Hex 20)

Command	Total No of Chars	Character Number												
		1	2	3	4	5	6	7	8	9	10	11	12	13
SetUnit														
Set Limits														
Set Ch A UL	13	^	S	L	A	U	1	.	2	3	4	sp	sp	sp
Set Ch A LL	13	^	S	L	A	L	0	.	7	8	9	sp	sp	sp
Set Ch B UL	13	^	S	L	B	U	1	.	2	3	4	sp	sp	sp
Set Ch B LL	13	^	S	L	B	L	0	.	7	8	9	sp	sp	sp
Set Computed UL	13	^	S	L	C	U	1	.	2	3	4	sp	sp	sp
Set Computed LL	13	^	S	L	C	L	0	.	7	8	9	sp	sp	sp
Set Measurement Type														
A	13	^	S	M	0	sp								
B	13	^	S	M	1	sp								
A+B	13	^	S	M	2	sp								
(A+B)/2	13	^	S	M	3	sp								
A-B	13	^	S	M	4	sp								
(A-B)/2	13	^	S	M	5	sp								
(B-A)a (angle)	13	^	S	M	6	sp								

7.0 RS232 User Input Commands (cont.)

7.1 RS232 User Command Details (cont.)

X = Value eg 3.4 pad with spaces

Command	Total No of Chars	Character Number												
		1	2	3	4	5	6	7	8	9	10	11	12	13
SetUnit														
Set Measurement Mode														
Track	13	^	S	O	N	sp								
Peak+	13	^	S	O	+	sp								
Peak-	13	^	S	O	-	sp								
Diff	13	^	S	O	D	sp								
Zero	13	^	S	Z	sp									
Peak Reset	13	^	S	P	E	A	K	R	E	S	E	T	sp	sp
Start Continuous Print	13	^	S	P	R	I	N	T	C	O	N	T	sp	sp
Stop Continuous Print	13	^	S	P	R	I	N	T	S	T	O	P	sp	sp
Set Print Key Single Mode	13	^	S	P	R	I	N	T	M	O	D	E	S	sp
Set Print Key Cont Mode	13	^	S	P	R	I	N	T	M	O	D	E	C	sp
Set I/O Logic State														
Logic Inputs Active Low	13	^	S	I	-	I	N	P	-	L	O	sp	sp	sp
Logic Inputs Active High	13	^	S	I	-	I	N	P	-	H	I	sp	sp	sp
Logic Outputs Active Low	13	^	S	I	-	O	U	T	-	L	O	sp	sp	sp
Logic Outputs Active High	13	^	S	I	-	O	U	T	-	H	I	sp	sp	sp
Notify														
Notify Probe Channel A	13	^	S	N	O	T	I	F	Y	-	C	H	A	sp
Notify Probe Channel B	13	^	S	N	O	T	I	F	Y	-	C	H	B	sp
Stop Notify	13	^	S	N	O	T	I	F	Y	H	A	L	T	sp
Zero Both	5	T	Z	0	0	0								
Zero One	5	T	Z	1	0	0								
Preset On	13	S	R	-	O	N	sp							
Preset Off	13	S	R	-	O	F	sp							
Set Preset Value	13	S	R	:	±	X	X	X	X	X	X	X	X	sp
Preset Toggle	13	S	R	-	T	O	G	G	L	E	sp	sp	sp	sp
Peak Reset	13	S	R	E	S	E	T	sp						

7.0 RS232 User Input Commands (cont.)

7.2 RS232 Output Formats

PRINT OUTPUT FORMATS

	0	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	
Format	C55 Compatible																				
Sign		Reading: right aligned, DP set by precision										Units				Limit	\n	\r			
Example	+0.00017mm	+			0	•	0	0	0	1	7			m	m			=	\n	\r	
	-0.0017mm	-			0	•	0	0	1	7				m	m			=	\n	\r	
	-0.017mm	-			0	•	0	1	7					m	m			=	\n	\r	
Format	NORMAL																				
Sign		Reading: right aligned, DP set by precision										Units				Limit	\n	\r			
Example	+1.1308mm	+					1	•	1	3	0	8			m	m			=	\n	\r
	-1.1308inch	-					1	•	1	3	0	8			i	n	c	h	=	\n	\r
	-1.1308	-					1	•	1	3	0	8							=	\n	\r
	-1.13mm	-					1	•	1	3					m	m			=	\n	\r

Note. XY print is not available when C55 'Print Mode' is selected. In this case only the selected channel will be printed.

Where:

- =space
- \r = CR
- \n = LF

7.0 RS232 User Input Commands (cont.)

7.2 RS232 Output Formats

EXTENDED	0	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21	22	23	24	25	26	27	28	29	30	31	32	33
Format	Sign	Reading, right aligned, DP set by precision												Units			Reading Type			Mode			r	\n										
+1.1308mm	+	1 • 1 3 0 8												m m			A B S			A			r	\n										
														i n c h			T A R E			B														
																	P R E			A + B														

The Extended Print is only available via remote RS232 commands (*P0 or *P1 or *P2). It is not selected, just requested.

XY mode	0	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21	22	23	24	25	26	27	28	29	30	31	32	33	34	35	36	37	38	39	40	41	42	43	44	45	46	47	48	49
Format	X :	Sign	Reading, right aligned, DP set by precision												Units			Limit	Y :	Sign	Reading, right aligned, DP set by precision												Units			Limit	r	\n												
X= +1.1308mm	X :	+	1 • 1 3 0 8												m m			>	Y :	-	2 • 4 2 1 5												m m			<	r	\n												
and over limit																																																		
Y= -2.4215mm																																																		
and under limit																																																		

Note. XY print is not available when C55 'Print Mode' is selected. In this case only the selected channel will be printed.

Where:
 =space
 r = CR
 \n = LF


8.0 Interface Connections

8.1 I/O CONNECTOR (Mounted on I/O Board)


25 WAY D TYPE SOCKET, FIXED TO REAR PANEL

PIN	DESCRIPTION	DETAIL
1	CH1 OVER RANGE	
14	CH1 IN RANGE	
2	CH1 UNDER RANGE	
15	CH2 OVER RANGE	
3	CH2 IN RANGE	
16	CH2 UNDER RANGE	
4	Isolated O/P Common	
17	'Zero key' Isolated I/P	
5	'Print key' Isolated I/P	
18	'Reset key' Isolated I/P	
6	'Peak key' Isolated I/P	
19	Log Control	
7	'Preset Enable'	
20	Isolated I/P Common	
8	Not Used	
21	Not Used	
9	Not Used	
22	Not Used	
10	Not Used	
23	CH1 Analogue O/P Common	CH1 O/P Return
11	CH1 Analogue O/P	CH1 Analogue O/P
24	CH2 Analogue O/P Common	CH2 O/P Return
12	CH2 Analogue O/P	CH2 Analogue O/P
25	Not Used	
13	Not Used	

Input Schematic



Output Schematic

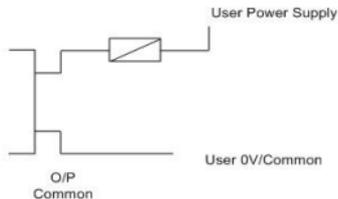

ANALOGUE OUTPUT SPECIFICATION	
Update interval	1.25mS
Bandwidth	500Hz
Rise time	70mS
Accuracy	0.1% FSO

8.0 Interface Connections (cont.)

8.2 COMMS CONNECTOR


9 WAY D TYPE PCB SOCKET, FIXED TO REAR PANEL

PIN	RS232 CONFIGURATION
1	Not Used
2	RS232 Tx
3	RS232 Rx
4	Not Used
5	RS232 GND
6	Not Used
7	Not Used
8	Not Used
9	Not Used

8.3 POWER CONNECTOR (Mounted on rear panel)

2.5 mm Chassis Mounted DC skt

PIN	DESCRIPTION	DETAIL
1	+24V DC Power IN(centre pin)	Power for Instrument routed through a switch
2	POWER RETURN	




8.0 Interface Connections (cont.)

8.4 Analogue Voltage and Current Inputs

12 way terminal block

12 Way Screen Terminal Strip Mounted on Rear Panel	
PIN	DESCRIPTION
1	+15V Output, 100mA Maximum
2	0V
3	-15V Output, 100mA Maximum
4	Channel A 4-20 mA Loop Source +
5	Channel A 4-20 mA Return
6	Channel A Voltage Input
7	Channel A Voltage Return
8	Channel B 4-20 mA Loop Source +
9	Channel B 4-20 mA Return
10	Channel B Voltage Input
11	Channel B Voltage Return
12	0V

Note: Pin 1 is to the right when viewed from rear

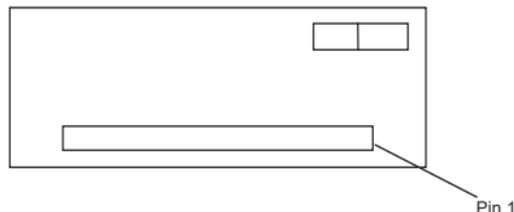

9.0 Technical Specification

MAIN INSTRUMENT	
Display Type	Colour LCD with integral backlight.
Display Length (mm)	±ABCD.EFGH
Display Length (inches)	±ABCD.EFGHJ
Resolution - Display	0.05µm or 0.000005"
Analogue Display	Solid Vertical bar
Keypad	9 key membrane keypad (Print, Zero, Peak/Track, Enter, Menu and navigation keys)
Temperature	Storage temperature range: -20°C to +85°C, Operating temperature range: 0°C to +50°C
IP Rating	Front panel: IP65, Case: IP51
POWER SUPPLY	
Voltage	+24V DC ±10%
Power	5 Watts maximum at 24V DC
(Universal 100-240V AC Input 24V DC PSU supplied with unit)	
MECHANICAL	
Weight	1.1kg excluding transducers
Dimensions	See drawing
ELECTRICAL CONNECTIONS (Rear Panel)	
DC Power	2.5mm DC Socket (Ctr pin +24V , Outer Return)
Input	2 x 4-20mA or 2 x DC Input
Serial Comms (RS232)	9 way D type socket
Input/Output	25 way D type socket
Digital Inputs	4 off switch activated with common isolated return
Digital Outputs	6 off current sink with common isolated return, programmable ACTIVE HI or LO Each pin can sink 500mA @ up to 40V
Analogue Outputs	1 for Channel A , 1 for Channel B, Independent Channel Range selection of : 0 to 5V, 0 to 10V, ± 5V, ± 10V, 4 to 20 mA - Accuracy 0.1% FSO